Installing your Agilent 8453E UV-visible Spectroscopy System

This is in your shipment

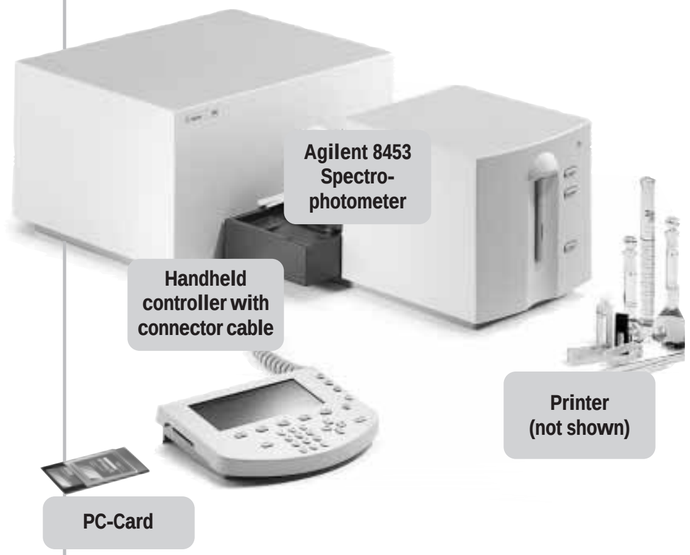

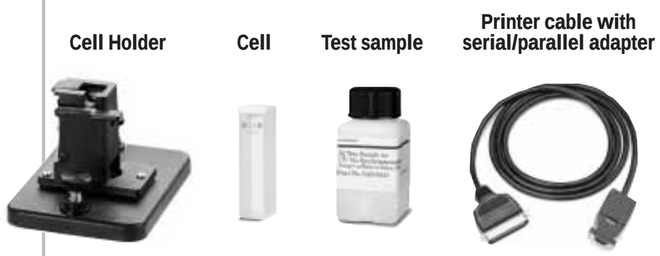

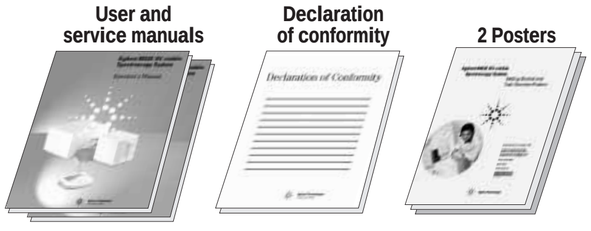

How you put your system together

Step 1:
Put the cell holder in the sample compartment and screw it down with the two fixing screws.

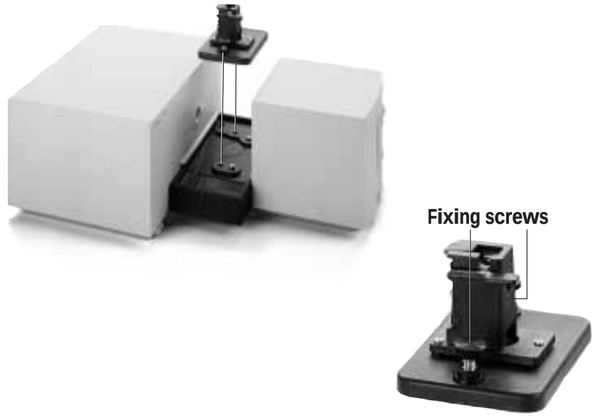

Step 2:
Connect the handheld controller to the spectrophotometer by plugging the connector cable into the right CAN interface at the rear of the spectrophotometer.

Step 3:
Connect the line power at the rear. The line voltage must be between 100 V and 240 V.

Step 4:
Install the printer according to the instructions in the printer's manual. Connect the printer to the RS 232 interface at the rear of the Agilent 8453 using the printer cable.

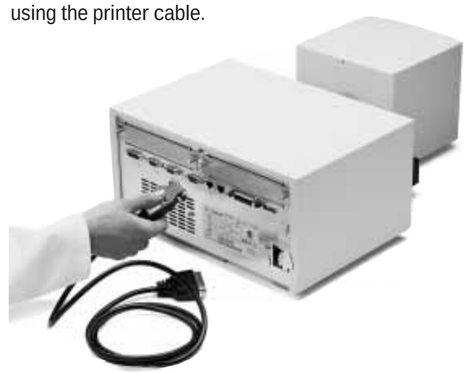

Step 5:
Turn on the spectrophotometer and handheld controller by pressing the power button of the spectrophotometer.

Step 6:
Turn on the printer by pressing the power button.

Now your system is setup and ready to use.

Agilent 8453E
UV-visible Spectroscopy System

Agilent Technologies